

RECEIVED

AUG 26 2002

TECH CENTER 1600/2900

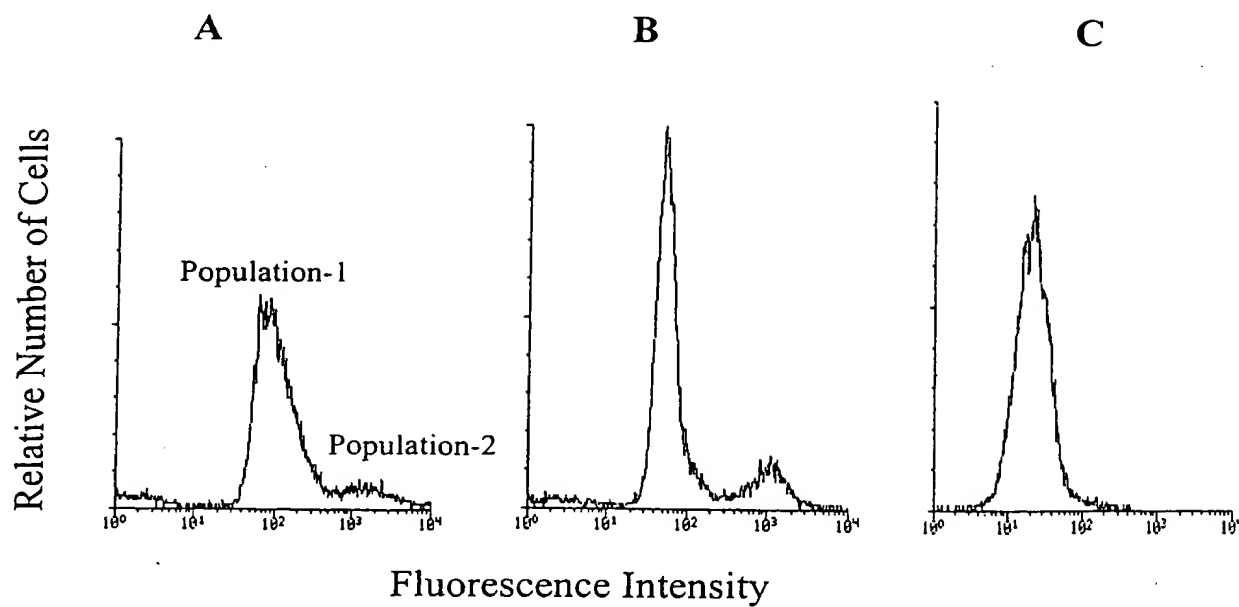


Fig. 2

RECEIVED

AUG 26 2002

TECH CENTER 1600/2900

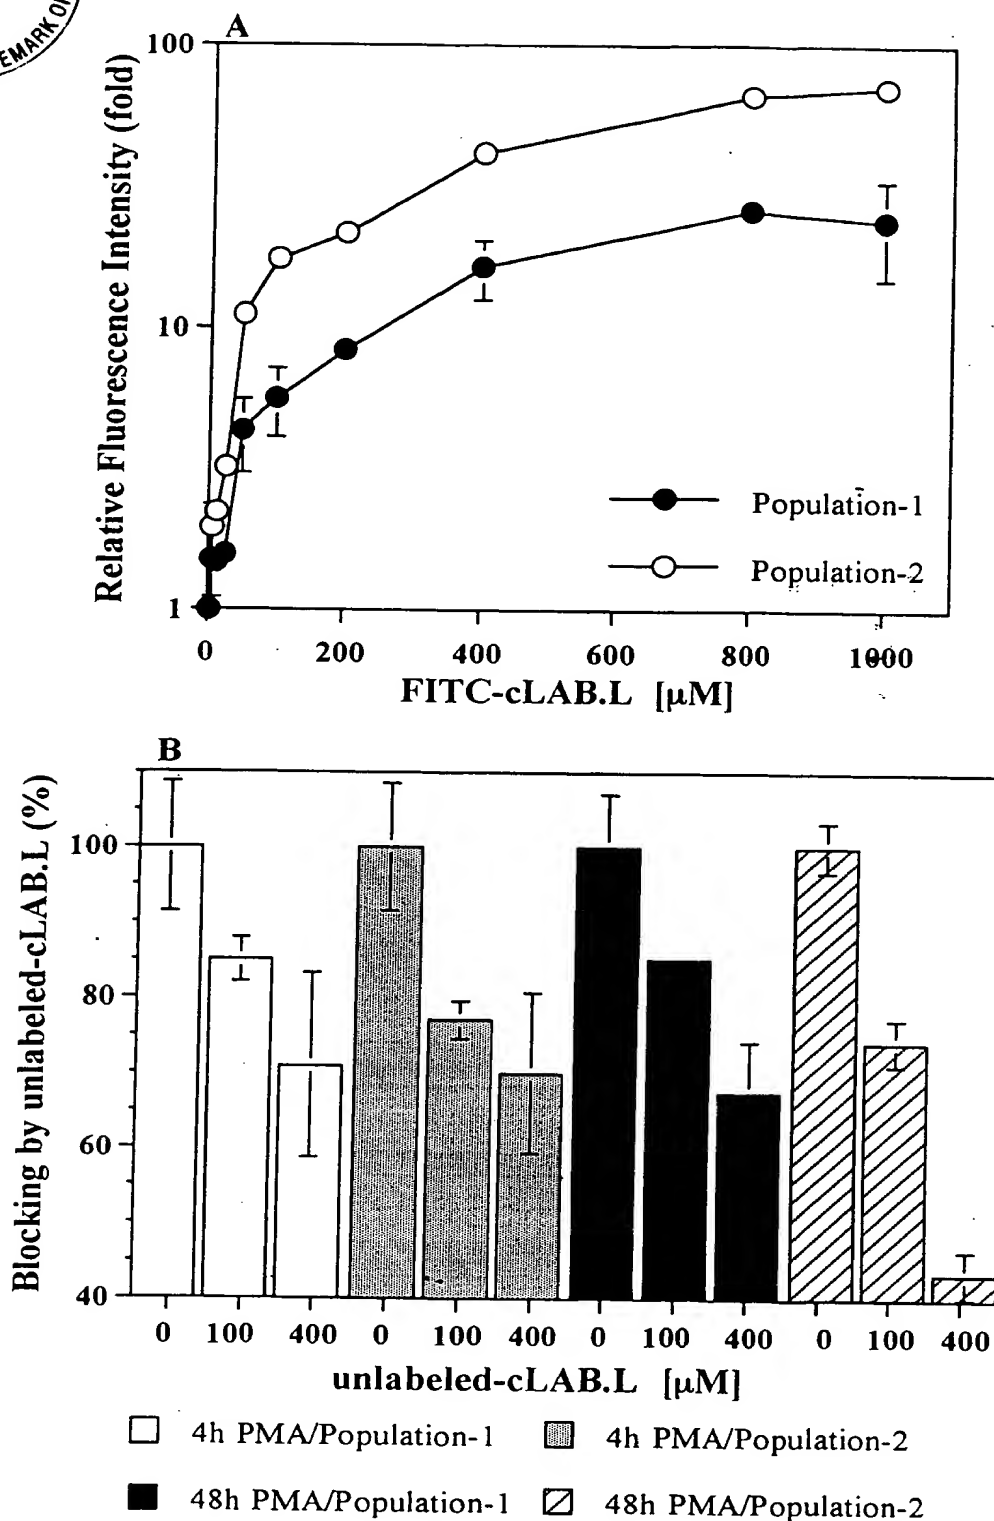
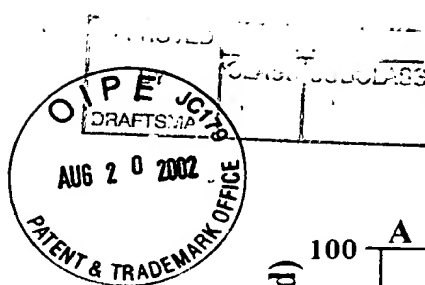


Fig. 3

AUG 26 2002

TECH CENTER 1600/2900



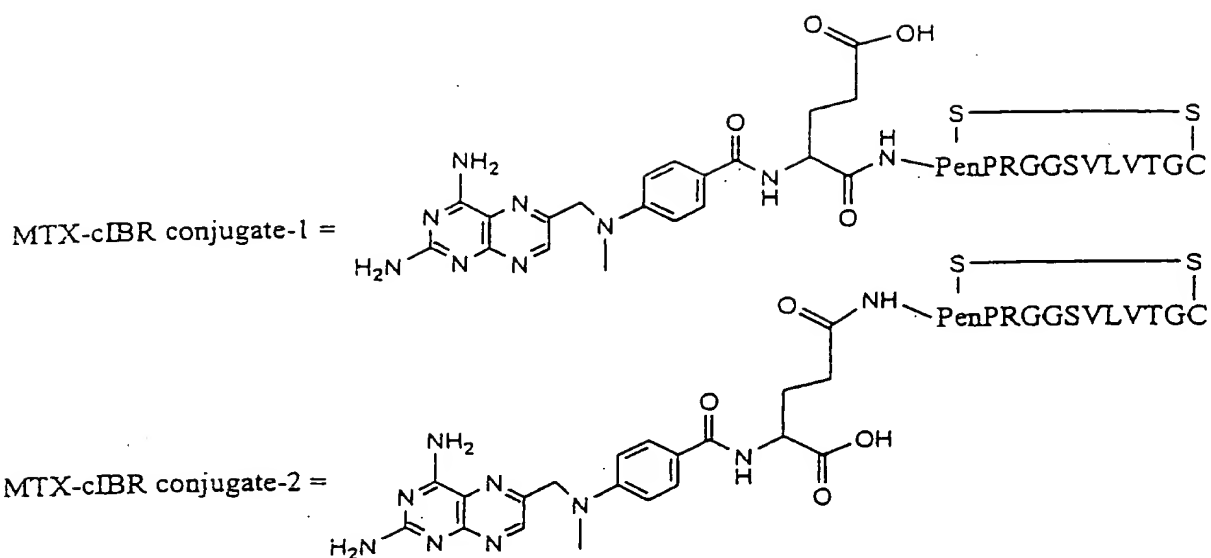


Fig. 7

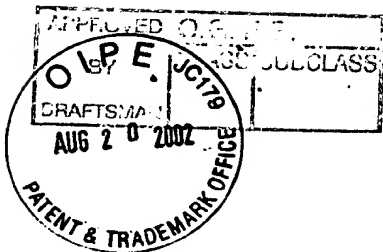

RECEIVED

AUG 26 2002

TECH CENTER 1600/2900

Toxicity of MTX-clBR by MTT assay

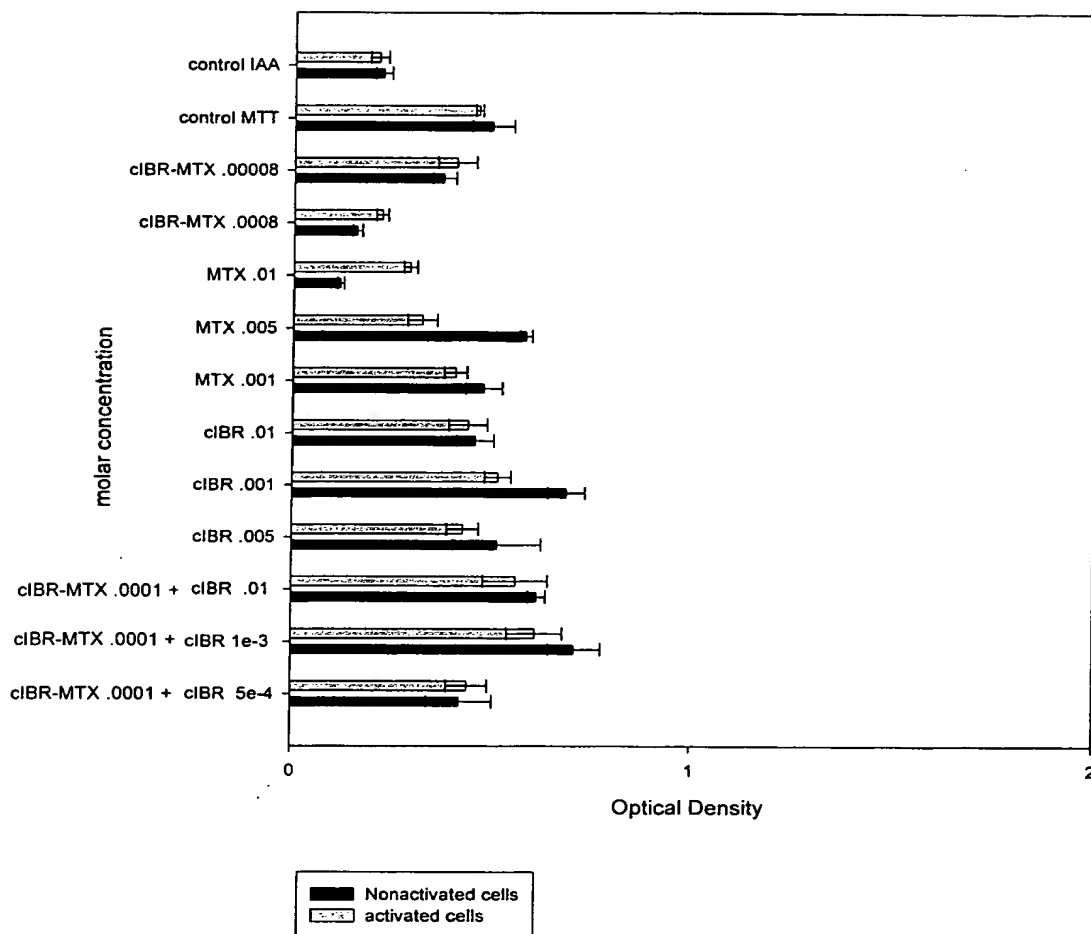


Fig. 9

RECEIVED

AUG 26 2002

TECH CENTER 1600/2900

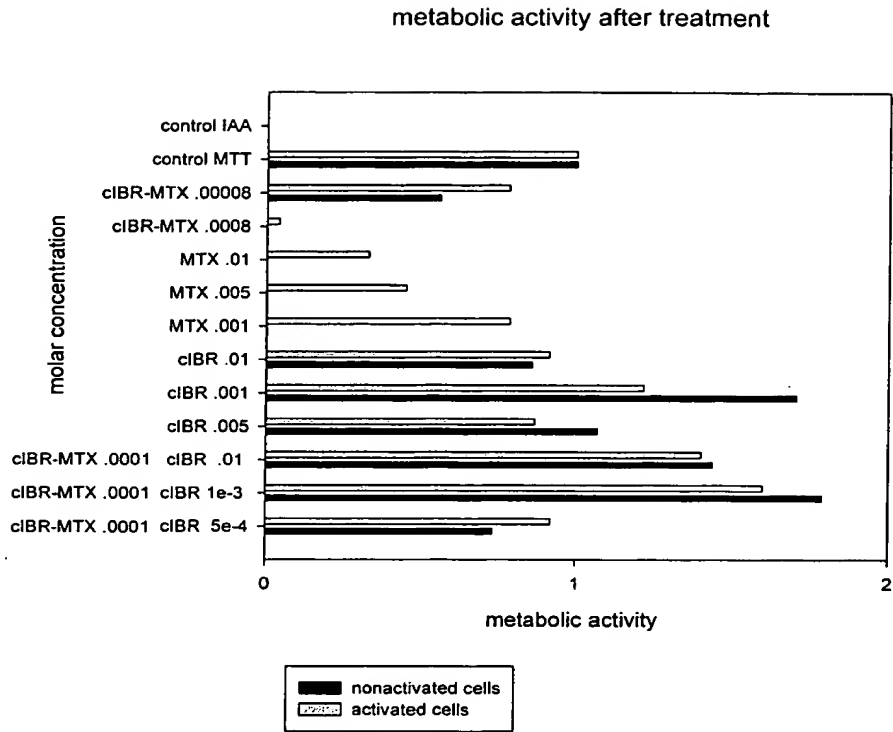
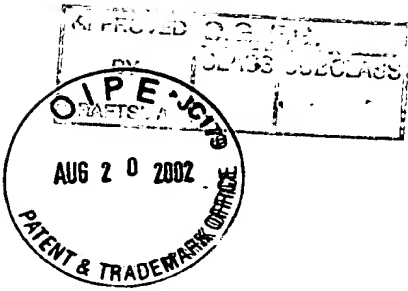


Fig. 10